



SERIES 501T



CARBON MONOXIDE ANALYZER OPERATION MANUAL




TABLE OF CONTENTS

SECTION	PAGE
• 1. About Nyad Carbon Monoxide Analyzer.....	3
• 2. Installation	4
• 3. The Sensor	5
• 4. The Electronics	6
• 5. Startup Display	8
• 6. Front Panel Controls	8
• 7. Activation "MENU"	9
• 8. Silencing Audible Alarm	10
• 9. Setting Alarm Points	12
• 10. Setting Analog and Digital Outputs	13
• 11. Default Values	14
• 12. Reference Menu	15
• 13. Cal Maint "One Touch Cal" Calibration Procedure	16
• 14. Replacing The CO Sensor	17
• 15. "Service" CO Sensor Replacement	18

(FIG 1)

NFPA COMPLIANT

The NYAD, Inc. Carbon Monoxide Analyzers meet or exceed CGA Grade-D specifications for air quality as adopted by Federal OSHA.

The NYAD, Inc. Carbon Monoxide Analyzers' quality standards meet or exceed OSHA 1910.134 requirements. When the components are used in accordance with the manufacturer's instructions and recommendations, the "analyzer" meets or exceeds federal regulations presently in force.

The NYAD, Inc. Carbon Monoxide Analyzer should be calibrated monthly and the Carbon Monoxide Sensor shall be replaced every 2 years for accuracy in accordance to the manufactures recommendation.

1) OSHA REGULATIONS (Standard-29 CFR)

Respiratory Protection 1910.134

2) 1910.134(i)(1)(ii)(C) Carbon monoxide (CO) content of 5—10 ppm or less.

NYAD, Inc. Carbon Monoxide Analyzer detection range is 0-2,000 ppm and is equipped with alarms when safe levels (5—10 ppm) are exceeded.



INTRODUCTION

Your CO analyzer is a self-contained unit capable of measuring the concentration of Carbon Monoxide. The range is 0 to 2,000 parts per million by volume (ppmv). The CO analyzer features two adjustable alarm contacts.

- Analog or digital (optional) signals with adjustable zero and span values and in addition to these features, a “One Touch Cal” auto-calibration function.

INSTALLATION

- a) Connect a regulated source of sample air to the 1/8” FNPT connection on the bottom of the enclosure labeled “INLET”. The inlet pressure should be between 15-20 psig. The recommended sample flow rate should be between .4 and .8 SCFH.
- b) Connect the instrument to a power source; 120/220 VAC 50/60 Hz, or 12VDC
- c) Turn the POWER switch to ON.

Note: Model COA-521T does not have a power switch.

- d) The CO analyzer will cycle through its diagnostic routine followed by current CO concentration value. The analyzer has been factory calibrated but a “bump” test should be performed to ensure accuracy.

QR CODE FOR
QUICK GUIDE
MISSING

THE SENSOR

The CO sensor is an electrochemical cell which has a life expectancy of about 2 years. Since the cell is an electrochemical device which is self-depleting, the cell output will gradually decrease as it is used.

LIFE EXPECTANCY:

APPROXIMATELY 6 MONTHS IN CONTAINER

APPROXIMATELY 3 YEARS IN AIR

RECOMMENDED REPLACEMENT INTERVAL EVERY 2 YEARS

THE ELECTRONICS

The electronics section of the NYAD Series 501T CO Analyzers is microprocessor based. The NYAD CO sensor produces a millivolt output. The signal enters the receiver section of the main electronic board which then shapes and amplifies the incoming signal and directs it to the microprocessor. The signal is amplified and converted to engineering units using memory-resident tables containing the relationship between signal and engineering units. The end product of this electronic process is displayed in terms of parts per million by volume (PPMV).

At this point, the processor performs three functions:

- 1) Allows for the two adjustable alarm contacts (SPDT relays).
- 2) Analog or Digital output signals.
- 3) Displays the measured values on a 4-digit LCD display.

Nyad offers two analog outputs:

- 0-5 volt DC or a
- 4-20mA current output

Other analog and digital outputs are available and can be factory set as 0-1VDC, RS232 or RS485. The zero point and span of these outputs are adjustable in the software




STARTUP ROUTINE

After the analyzer has been installed, all electrical connections have been made and power turned on, the instrument will proceed through its power-up routine with the display and indicators stepping through the following sequence:

- a) Displays all segments ON and all LED indicators ON for one second. This step verifies the operation of those devices.
- b) Displays the word NYAD for one second.
- c) The display indicates the version of the current operating system software.

All LED indicators are off followed by INT and CO.

The last step in the startup routine is the display of the current CO value. In approximately six seconds, any alarm conditions will be shown on AL1 and/or AL2 red LED alarm indicator and the audible alarm will sound.

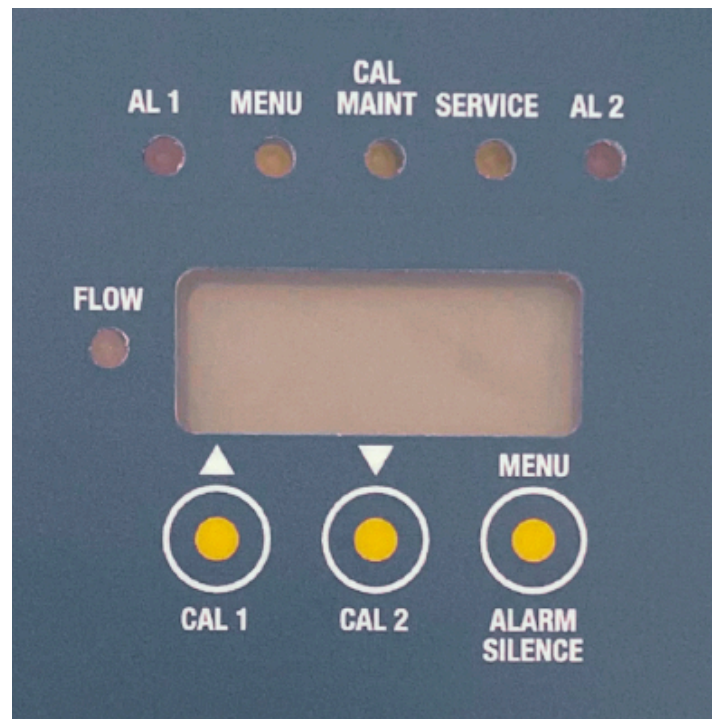

FRONT PANEL CONTROLS

1) UP Arrow and DOWN Arrow Button

- a) Changes the value of set point, outputs, and constants.
- b) Changes the calibration values.
- c) Changes toggle function "Hi and Lo"

2) **CAL 1** - This button is used during "One Touch Cal" calibration process using 10 ppm CO span gas.

3) **CAL 2** - This button is used during "One Touch Cal" calibration process using 20 ppm CO span gas.

4) **MENU** - Pressing the MENU button allows the operator to view the current settings. Pressing and holding the MENU button allows the operator to have access, interrogate, and reset the other major functions incorporated into this analyzer, namely, Alarm 1 and 2, Outputs, Toggles, Factory Codes and Calibration settings.

5) **ALARM SILENCE** - This button is used to temporarily silence the audible alarm. The audible alarm will automatically reactivate in 10 minutes

AL1 Red LED Alarm 1 indicator will illuminate indicating the CO value has exceeded Alarm 1 set-point value.

MENU Yellow LED indicator

- Solid Yellow - MENU disabled. Available for viewing current settings only
- Slow Blinking Yellow - "ONE TOUCH CAL" enabled. User in calibration mode.
- Fast Blinking Yellow - MENU enabled. User access available.

CAL MAINT Yellow LED indicator will illuminate indicating calibration is required.

SERVICE Yellow LED indicator will illuminate indicating CO sensor replacement is required.

AL2 Red LED Alarm 2 indicator will illuminate indicating the CO value has exceeded Alarm 2 set-point value.



FLOWLIGHT

NYAD model COA-501T is equipped with a flowmeter which allows the user to visually see the rate of flow in SCFH.

- Recommended flow rate is between .4 to .8 SCFH.

ACTIVATION MENU

In normal operations, the MENU button is disabled. The user will only be able to view the current settings set by the factory. To change factory settings such as Alarm 1 and Alarm 2 set-points, Outputs Hi and Lo, the “MENU” must be activated by a Certified Technician

To activate the “MENU”

- 1) Press and hold the MENU button for about 10 seconds until CODE is displayed. The MENU LED will begin to blink fast. Press the DOWN arrow button to change the value to 135.
- 2) Press the MENU button to the desired location and use the UP arrow or DOWN arrow button to change settings.

Note: Once changes are made, the display will automatically default in about 10 seconds, flash “CO” and return to the current measure CO value. Also, once you scroll through the entire menu, the display will automatically default and return to normal operations).



SILENCING AUDIBLE ALARM

To silence the audible alarm, press the “ALARM SILENCE” button once. The audible alarm will be temporarily disabled and will automatically reactivate in 10 minutes.

SETTING ALARM POINTS

This analyzer has two adjustable alarm set points and relays as factory standard. When the measured value of CO concentration exceeds the set point for a sustained period of about 6 seconds, the alarm condition will become activated. The SPDT relay (Alarm 1) is energized as is the red front-panel LED indicator, AL1.

To determine the current setting for ALARM 1, press the MENU button. The display will show AL1 and then default to the current value. If this value is acceptable, the display will automatically default in about 10 seconds and flash "CO" and return to the current measured CO value.

To change ALARM 1 (AL 1) set-point the "MENU" must be activated by a Certified Technician as described in Section 7.

- a) Press and hold the MENU button for about 10 seconds until CODE is displayed. The MENU LED will begin to blink fast. Press the DOWN arrow button to change the value to 135.
- b) Press the MENU button, AL 1 will momentarily display followed by the current Alarm 1 set-point value. Press the UP arrow or DOWN arrow to change Alarm 1 value.

To change ALARM 2 (AL 2) set-point, proceed exactly as described above after pressing the MENU button to display AL2 and its current value.

If the measured value of CO concentration is higher than the ALARM 1 or ALARM 2 settings, the corresponding LED will illuminate above the display and energize the alarm relay thus activating any warning devices connected to it.

ALARM TOGGLE POINTS

NYAD Series 501T Analyzers are equipped with a toggle function (A1 1t and A2 2t). Set these “Hi” when detecting increasing CO and “Lo” when detecting decreasing CO

- To view the current setting for AL 1t, press the MENU button two times.

FACTORY DEFAULTS

AL 1t	Hi
AL 2t	Hi

- The display will show AL 1t followed by Hi or Lo.
- Press the MENU button two or more times, AL 2t will displayed followed by Hi or Lo.
- If these settings are acceptable, the display will automatically default in about 10 seconds, flash "CO" and return to the current measured CO value.

SETTING ANALOG AND DIGITAL OUTPUTS

The NYAD Series 501T Analyzers features a 0-5 VDC and 4-20mA analog output as factory standard. This signal is linearly proportional to ppm CO. To view the current output settings:

- a) Press the MENU button five times. “oPHi” will be displayed. The display will then show the CO concentration (50 ppm default) corresponding to the Hi end (5 VDC) of the analog output scale.
- b) Press the MENU button more one time, the display will now read “oPLo” and then show the CO concentration (0 ppm default) corresponding to the Lo end (0 VDC) of the analog output scale.

The RS-485 option uses a 25' 3 wire cable Red, Green, Black.

A = Red

B= Green

Ground = Black

To activate the digital output, the “MENU” must be activated by a Certified Technician as described in Section 7.

To change span values from those set at the factory, the “MENU” must be activated by a Certified Technician as described in Section 7. “Activation Menu”.

a) Press and hold the MENU button for about 10 seconds until CODE is displayed. The MENU LED will begin to blink fast. Press the DOWN arrow button to change the value to 135.

DIGITAL OUTPUT

The NYAD Series 501T Analyzers features an optional digital output port. The user has a choice of format, either RS-232 or RS-485.

The RS-232 option can be accessed from a standard DB-9 connector located on the bottom of the enclosure or rear panel.

ACTIVATING RS232

- a) Press and hold the MENU button for about 10 seconds until CODE is displayed. The MENU LED will begin to blink fast. Press the UP arrow button to change the value to 159.
- b) Press the MENU button nine times. The display will show PORT. Press the UP or DOWN arrow and select 0232 (RS232) or 0485 (RS4850). Press the MENU seven times. The display will default back to the current measured CO value or in about 10 seconds, the display will automatically default, flash "CO" and return to the current measured CO value.

The digital output is now activated and a constant data stream will be sent every second with the following information:

Data Output format:

\$UNITS, Display_data, Output, ALARM1, ALARM2,
ERROR#1, Line_checksum<CR><LF>

EXAMPLE: \$CO, 1.4, 0.238, 0, 0, 0, 1177<CR><LF>

DEFAULT VALUES

Series 501T Analyzers are preset at the factory with the following standard values:

- Function PPMV
- Al 1 5
- Al 2 10
- Output (oPHi) 50
- Output (oPLo) 00

These settings can be changed to values most suitable for your application.

REFERENCE MENU

AL1	Dry Relay Contact - Alarm 1
AL2	Dry Relay Contact -- Alarm 2
Al 1t	Toggle Alarm 1 "Hi or Lo"
A2 2t	Toggle Alarm 2 "Hi or Lo"
OpHi	Analog Output "Hi"
OpLo	Analog Output "Lo"
CAL 1	Calibration using 10 ppm span gas
CAL 2	Calibration using 20 ppm span gas
CAL	CAL "One Touch Cal" Calibration Mode
No LEL	Sensor not detecting CO
EroP	Operator Error

CAL MAINTENANCE - “One Touch Cal”



WARNING

High carbon monoxide concentrations are toxic. Take appropriate ventilation precautions when calibrating with a span gas.

CALIBRATION PROCEDURE

Calibration interval should be carried out once a month and can be performed by a non-certified technician. The “Cal Maintenance” LED will illuminate indicating calibration is required.

To calibrate the CO sensor use a certified sample 10 ppm or 20 ppm CO span gas balanced in air. The calibration gas concentration can be changed in the menu settings if you are using anything other than 10 ppm or 20 ppm span gas.

To begin the “One Touch Cal” calibration process:

- 1) Turn sample air off.
- 2) Attach 10 or 20 PPM CO span gas to the Calibration Port. If using a gauge, start the flow rate between 200 and 500 cc/min. (Refer to the gauge on the gas cylinder and not the flow meter on the analyzer). Allow the displayed CO value to stabilize to a constant value. If a gauge is not being used, the flowmeter on the panel can be referenced. Turn on the flow and adjust until the flowmeter shows between .4 and .8 SCFH/.

- 3) To activate the “One Touch Cal”, press and hold the MENU button for 5 seconds, “CAL” will momentarily display followed by the current CO value.

The MENU LED will start blinking.

- 4) Select “One Touch Cal” CAL 1 or CAL 2. The display will show CAL 1 for 10 ppm or CAL 2 for 20 ppm followed by CO 10 or CO 20.

The MENU LED will stop blinking and the CAL MAINT LED will now turn off.

- 5) Turn off and remove span gas. Allow 5-10 minutes for the CO value to return to zero.

To disable “One Touch Cal” while in calibration mode, press and hold the MENU button for 5 seconds. The MENU LED will stop blinking and the analyzer will momentarily default back to the current measured CO value.

CALIBRATING WITH OTHER CO SPAN GASES:

To use CO span gases other than 10 ppm or 20 ppm, the “MENU” must be activated by a Certified Technician as described in Section 7. “Activation Menu”.

- a) Press and hold the MENU button for about 10 seconds until CODE is displayed. The MENU LED will begin to blink fast. Press the UP arrow button to change the value to 159.
- b) Press the MENU button seven times. The display will show CAL2 followed by 20. Change the value to the desired gas value by using the UP arrow or DOWN arrow button.
- c) Press the MENU button nine times, the display will default back to the current measured CO value or in about 10 seconds, the display will automatically default, flash “CO” and return to the current measured CO value.

Begin the calibration process using “One Touch Cal” CAL 1 or CAL 2 as described in Section 13: “Calibration Procedure”.

REPLACING THE CO SENSOR

- 1) Remove the plastic cover on model COA-551T or chassis cover on models COA-531T and COA-551T.
- 2) Remove the front panel (two thumb screws on model COA-551T).
- 3) Carefully pull the complete sensor module counter clock wise it is free of the input fitting
- 4) Remove the electronic board from the assembly by pulling it away from the sensor where it is held by three connector pins. Next remove the sensor from its flow chamber by unscrewing the three small screws holding it in place. Discard the depleted cell and replace it with the new one.
- 5) Reassemble the cell by following the above instructions in reverse.



DANGER

Disconnect power to the unit before performing any maintenance to the control board



WARNING

The CO sensor contains corrosive acid. Do not attempt to open. Before disposing of sensor place it in a polyethylene bag and tie securely. Dispose of sensor in accordance with all applicable regulations.

“Service” - CO SENSOR REPLACEMENT

The Nyad CO sensor should be replaced every two years and should be performed by a Certified Technician. The “Service” LED will illuminate indicating when the CO sensor replacement is required.

After replacing the CO sensor, the Service LED indicator must be reset. To reset, the “MENU” must be activated by a Certified Technician as described in Section 7. Activation Menu.

- a) Press and hold the MENU button for about 10 seconds until CODE is displayed. The MENU LED will begin to blink fast. Press the UP arrow button to change the value to 159.
- b) Press the MENU button 10 times, the display will show “SSer”. Press the UP arrow button to change the value to 1.
- c) The “Service” LED will now turn off.
- d) The sensor is now ready for calibration. Ø Refer to Section 13. Calibration Procedure

NOTE: CALIBRATION IS REQUIRED AFTER REPLACING THE CO SENSOR.



CARBON MONOXIDE DANGER LEVELS

Levels of Carbon Monoxide are considered dangerous.
The chart below shows the health effects of CO exposure.

CO concentration (parts per million)	SYMPTOMS
50	No adverse effects with 8 hours of exposure
200	Mild headache after 2-3 hours of exposure
400	Headache and nausea after 1-2 hours of exposure.
800	Headache, nausea, and dizziness after 45 minutes; collapse and loss of consciousness after 1 hour of exposure.
1,000	Loss of consciousness after 1 hour of exposure
1,600	Headache, nausea, and dizziness after 20 minutes of exposure
3,200	Headache, nausea, and dizziness after 5-10 minutes; collapse and loss of consciousness after 30 minutes of exposure
6,400	Headache and dizziness after 1-2 minutes; loss of consciousness and danger of death after 10- 15 minutes of exposure
12,800	Immediate physiological effects, loss of consciousness and danger of death after 1-3 minutes of exposure

THE US STANDARDS FOR CO LEVELS ARE AS FOLLOWED

Maximum of 35 ppm of CO for 1-hour exposure:

- Ø Not to be exceeded more than once per year.

Maximum of 9 ppm of CO for 8-hour exposure:

- Ø Not to be exceeded more than once per year

SPECIFICATIONS

MODEL NUMBER	COA-221T (OEM), COA-231T (RACK MOUNT), COA-241T (PANEL MOUNT), COA-251TS (NEMA 4), COA-2717T (NEMA-7X)	
UNITS	PPM (Parts Per Million)	
STANDARD	Display	Backlit 4 Digit LCD, 0.5" High
	Alarm	Dual Dry Relay Contacts (SPDT 1A@120V)
	Analog Output	0-5VDC or 4-20mA (Adjustable zero and span)
	Power	120/220VAC
		50/60 Hz, 1W Max
	Memory	Non-Volatile Data Memory
	Inlet	1/8" FNPT
	Calibration	"One Touch Cal" Auto Calibration
	Audible Alarm	95 db, frequency 2700 to 3700 Hz
	Mini-Rate Flowmeter	0-1.0 SCFH
OPTIONS	Digital Output	RS232, RS485
	Power	12V
SENSOR	Response Time	90% in 30 seconds
	Operating Humidity	15 to 90% RH non-condensing
	Inlet Pressure	30-35 lbs MAX
	Operating Temperature	-20°C to +50°C
	Sensor Life in Air	Up to 24 Months at 30°C
	Sensor Shelf Life	1 Year
	Replacement	Every 2 years
	Sensor Warranty	1 Year
	Calibration Gas	CO span gas balance air
	Calibration Interval	Once a month
	Sample Flow	Between and .4 and .8 SCFH or 200-500 cc/min

ENCLOSURES

OEM	5.75"W x 6.75"H x 2.4"D
NEMA-4	7.72"Wx7.72"Hx5.71"D
PANEL	10"W x 6.25"H x 6"D
RACK	19"W x 5.25"H x 6"D
NEMA-7X	8.37"W x 9.87"H x 6.53"D

TROUBLESHOOTING GUIDE

SYMPTOMS	REMEDY
ELECTRONICS Unit will not cycle Startup routine not normal Display is blank with power on Display has missing segments	Please contact NYAD for verbal evaluation. Unit will likely need to be sent to NYAD for further evaluation.
ERROR CODES ErOp (Error Operator) E-Lo No LEL	Output out of range. Set output Lo and Hi. See Section 10 Setting Output. Replace CO sensor or CO round electronics. Sensor not detecting CO Gas. Make sure all connections are secure. Replace CO sensor

WARRANTY

WARRANTY TERMS

Nyad, Inc. warrants to the original consumer purchaser that all parts used in the construction or fabrication of the Nyad Equipment will be free from defects in materials and factory workmanship, under normal use and service for five years from the date of delivery.

Warranty coverage provides the necessary repairs or parts replacement found by Nyad, Inc. to be defective due to bad workmanship or faulty materials.

LIMITATIONS OF WARRANTY

The Nyad Equipment is restricted to inspection (FOB the Factory) before warranty is determined, unless other arrangements have been made by Nyad and the original consumer purchaser.

This warranty does not apply to routine service/maintenance, repairs and routine calibration of the moisture sensor every twelve (12) months in accordance with manufacturer's recommendation, or replacements made necessary by fire or water damage, or accident to or improper installation by others, alteration, misuse or abuse to the Nyad Equipment.

This warranty does not cover labor charges or cost incurred for time and expense by other service agencies or personnel involved in maintaining the Nyad Equipment.

Application of this Warranty is further conditioned upon the following:

Installation. The Nyad Equipment must be properly installed in accordance with Nyad's installation procedures and instructions.

Proper Maintenance and Operation. The Nyad Equipment must be properly maintained and operated in accordance with Nyad's maintenance and operating procedures. All service parts must be acquired from Nyad or its authorized representative.

No Alteration. The Nyad Equipment must not have been modified or altered from its original conditions at the date of delivery or installation.

Failure to comply with any of these conditions will void this Warranty

RETURN POLICY

Before returning any items (except for recalibration service and repairs) you must call 925 270-3971 8:30 a.m. – 5:00 p.m. PST. Monday through Friday for approval.

Product may be returned for a full refund/credit within 30 days from the date that Nyad originally shipped and must be returned in their original new condition. Exceptions for special order. Returns for special orders will have 30% restocking fee and must be approved.

Items returned in damaged or altered conditions which cannot be resold as new will have a 30% restocking fee.

All returned items are subject to inspection for use and damage before credit is issued. Returns may incur additional charges if product is returned in damaged conditions.

Manufacture Warranty/Defective Claims - You may return product to us for rework, exchange and/or request a full refund/credit. Request must be made from the original purchaser. Upon receipt of a returned item, Nyad will evaluate and determine the warranty claim.

Damaged Items – It is your responsibility to inspect your packages for damages/defect on delivery. If product is damaged in transit to you, we must be notified immediately (within 24 hours) so that we can submit a claim to our freight carrier.

Lost Packages – Lost Packages must be reported within 30 days of shipment date and verification from the freight carrier that product has not been delivered.

Please contact or email us for further important instructions on filing a lost or damaged package claim

TECHNICAL SUPPORT

Nyad, Inc. will offer Technical Support via telephone or email. All technical support shall be related to the Nyad Equipment only. Any other technical issues involving other products and services to the Nyad Equipment will not be the responsibility of Nyad, Inc.; however, our technical support team will offer their best knowledge and support involved in the Nyad Equipment.

Warranty/Technical Support:

Ph (925) 270-3971

Contact: Carissa Harrild

Email: sales@nyad.com

www.nyad.com